



# DC Power Supply

GPD-X303S Series

---

## USER MANUAL

PART NO. 82PD-433SoMo1



ISO-9001 CERTIFIED MANUFACTURER

This manual contains proprietary information, which is protected by copyrights. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Combined Test Solutions.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

# Table of Contents

**SAFETY INSTRUCTIONS** ..... 5

**OVERVIEW**..... 10

- Introduction..... 10
- Series Lineup / Main Features ..... 13
- Principle of Operation..... 14
- Front Panel Overview ..... 16
- Rear Panel Overview ..... 21
- CV/CC Crossover Characteristics ..... 22

**SETUP**..... 23

- Power Up ..... 23
- Load Cable Connection ..... 24
- Output On/Off..... 25
- Beep On/Off ..... 25
- Switch between channels ..... 26
- Front Panel Lock ..... 26

**OPERATION**..... 27

- CH1/CH2 Independent Mode ..... 27
- CH3 Independent Mode..... 29
- CH4 Independent Mode..... 31
- CH1/CH2 Tracking Series Mode..... 33
- CH1/CH2 Tracking Parallel Mode ..... 39

**SAVE/RECALL SETUP** ..... 41

- Save Setup ..... 41
- Recall Setup..... 42

**REMOTE CONTROL** ..... 43

- Remote Control Setup..... 43

|                                |           |
|--------------------------------|-----------|
| Remote Connection Step.....    | 44        |
| Command Syntax .....           | 46        |
| Error Messages .....           | 46        |
| Command List.....              | 47        |
| Command Details .....          | 48        |
| <b>FAQ .....</b>               | <b>53</b> |
| <b>APPENDIX .....</b>          | <b>54</b> |
| Fuse Replacement .....         | 54        |
| Specifications .....           | 55        |
| Declaration of Conformity..... | 57        |
| <b>INDEX.....</b>              | <b>58</b> |

# S SAFETY INSTRUCTIONS

This chapter contains important safety instructions that you must follow when operating the GPD-X303S series and when keeping it in storage. Read the following before any operation to insure your safety and to keep the best condition for the GPD-X303 series.

## Safety Symbols

These safety symbols may appear in this manual or on the GPD-X303S series.

---



**WARNING**

Warning: Identifies conditions or practices that could result in injury or loss of life.



**CAUTION**

Caution: Identifies conditions or practices that could result in damage to the GPD-X303S series or to other properties.



**DANGER High Voltage**



Attention Refer to the Manual



Protective Conductor Terminal



Earth (ground) Terminal



Do not dispose electronic equipment as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased.

## Safety Guidelines

---

### General Guidelines



#### CAUTION

- Do not place any heavy object on the GPD-X303S series.
- Avoid severe impacts or rough handling that leads to damaging the GPD-X303S series.
- Do not discharge static electricity to the GPD-X303S series.
- Do not block or obstruct the cooling fan vent opening.
- Do not perform measurement at circuits directly connected to Mains (see note below).
- Do not disassemble the GPD-X303S series unless you are qualified as service personnel.

(Measurement categories) EN 61010-1:2001 specifies the measurement categories and their requirements as follows. The GPD-X303S series falls under category I.

- Measurement category IV is for measurement performed at the source of low-voltage installation.
- Measurement category III is for measurement performed in the building installation.
- Measurement category II is for measurement performed on the circuits directly connected to the low voltage installation.
- Measurement category I is for measurements performed on circuits not directly connected to Mains.

---

### Power Supply



#### WARNING

- AC Input voltage: 100V/120V/220V/230V ±10%, 50/60Hz
  - Connect the protective grounding conductor of the AC power cord to an earth ground, to avoid electrical shock.
-

Fuse



WARNING

- Fuse type: 100V/120V: T6.3A/250V, 220V/230V: T3.15A/250V
  - Make sure the correct type of fuse is installed before power up.
  - To ensure fire protection, replace the fuse only with the specified type and rating.
  - Disconnect the power cord before fuse replacement.
  - Make sure the cause of fuse blowout is fixed before fuse replacement.
- 

Cleaning the  
GPD-X303S  
series

- Disconnect the power cord before cleaning.
  - Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid.
  - Do not use chemicals or cleaners containing harsh products such as benzene, toluene, xylene, and acetone.
- 

Operation  
Environment

- Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (note below)
  - Relative Humidity: < 80%
  - Altitude: < 2000m
  - Temperature: 0°C to 40°C
-

(Pollution Degree) EN 61010-1:2001 specifies the pollution degrees and their requirements as follows. The GPD-X303S series falls under degree 2.

Pollution refers to “addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity”.

- Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence.
- Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected.
- Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.

---

### Storage environment

- Location: Indoor
- Relative Humidity: < 70%
- Temperature: -10°C to 70°C

---

### Disposal



Do not dispose this instrument as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased. Please make sure discarded electrical waste is properly recycled to reduce environmental impact.

### Power cord for the United Kingdom

When using the GPD-2303S/GPD-3303S/GPD-4303S series in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead/appliance must only be wired by competent persons



**WARNING: THIS APPLIANCE MUST BE EARTHED**

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

|                |              |
|----------------|--------------|
| Green/ Yellow: | Earth        |
| Blue:          | Neutral      |
| Brown:         | Live (Phase) |



As the colours of the wires in main leads may not correspond with the colours marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with the letter E or by the earth symbol  $\oplus$  or coloured Green or Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, cable of 0.75mm<sup>2</sup> should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any moulded mains connector that requires removal /replacement must be destroyed by removal of any fuse & fuse carrier and disposed of immediately, as a plug with bared wires is hazardous if a engaged in live socket. Any re-wiring must be carried out in accordance with the information detailed on this label.

# VERVIEW

This chapter describes the GPD-2303S/GPD-3303S/GPD-4303S series in a nutshell, including its main features and front / rear panel introduction. After going through the overview, follow the Setup chapter (page23) to properly power up and set operation environment.

## Introduction

---

### Overview

The GPD-X303S regulated DC power supply series are light weight, adjustable, multifunctional work stations. The GPD-2303S has a 2 independent adjustable voltage outputs. The GPD-3303S three independent outputs: two with adjustable voltage levels and one with fixed level selectable from 2.5V, 3.3V and 5V. The GPD-4303S has four independent voltage outputs that are all fully adjustable. The GPD-X303S series can be used for logic circuits where various output voltage or current are needed, and for tracking mode definition systems where plus and minus voltages with insignificant error are required.

---

Independent / Tracking Series / Tracking Parallel      The three output modes of GPD-X303S series, independent, tracking series, and tracking parallel, can be selected through pressing the TRACKING key on the front panel. In the independent mode, the output voltage and current of each channel are controlled separately. The isolation degree, from output terminal to chassis or from output terminal to output terminal, is 500V. In the tracking modes, both the CH1 and CH2 outputs are automatically connected in series or parallel; no need to connect output leads. In the series mode, the output voltage is doubled; in the parallel mode, the output current is doubled.

Constant Voltage/ Constant Current      Each output channel is completely transistorized and well-regulated, and works in constant voltage (CV) or constant current (CC) mode. Even at the maximum output current, a fully rated, continuously adjustable output voltage is provided. For a big load, the power supply can be used as a CV source; while for a small load, a CC source. When in the CV mode (independent or tracking mode), output current (overload or short circuit) can be controlled via the front panel. When in the CC mode (independent mode only), the maximum (ceiling) output voltage can be controlled via the front panel. The power supply will automatically cross over from CV to CC operation when the output current reaches the target value. The power supply will automatically cross over from CC to CV when the output voltage reaches the target value. For more details about CV/CC mode operation, see page22.

---

Automatic tracking mode      The front panel display (CH1, CH2) shows the output voltage or current. When operating in the tracking mode, the power supply will automatically connect to the auto- tracking mode.

---

Dynamic load      When used in audio production lines, the power supply can provide a continuous or dynamic load using a jumper connector (JP101/JP401). When the jumper connectors are connected to the “ON” position (shorted), a stable DC current power will be provided for audio power amplifiers.

---

## Series Lineup / Main Features

### Main Features

---

|             |  |
|-------------|--|
| Performance | <ul style="list-style-type: none"><li>• Low noise: Temperature controlled cooling fan</li><li>• Compact size, light weight</li></ul>   |
| Operation   | <ul style="list-style-type: none"><li>• Constant Voltage / Constant Current operation</li><li>• Tracking Series / Tracking parallel operation</li><li>• Output On/Off control</li><li>• Multi-output:<br/>GPD-2303S: 30V/3A x2;<br/>GPD-3303S: 30V/3A x2, 2.5V/3.3V/5V/3A x 1<br/>GPD-4303S: 30V/3A x2, 5V/1A x1, 5V/3A<br/>(10V/1A) x1</li><li>• Digital panel control</li><li>• 4 sets of panel setup save/recall</li><li>• Coarse and fine Voltage/Current control</li><li>• Software calibration</li><li>• Buzzer output</li><li>• Key lock function</li></ul> |
| Protection  | <ul style="list-style-type: none"><li>• Overload protection</li><li>• Reverse polarity protection</li><li>• Overvoltage protection</li></ul>   |
| Interface   | <ul style="list-style-type: none"><li>• USB for remote control</li></ul>   |

## Principle of Operation


### Overview

The power supply consists of the following.

- AC input circuit
- Transformer
- Bias power supply including rectifier, filter, pre-regulator and reference voltage source
- Main regulator circuit including the main rectifier and filter, series regulator, current comparator, voltage comparator, reference voltage amplifier, remote device and relay control circuit


The block diagram below shows the circuit arrangement. The single phase input power is connected to the transformer through the input circuit. Details of each part are described in the next page.

### Block diagram

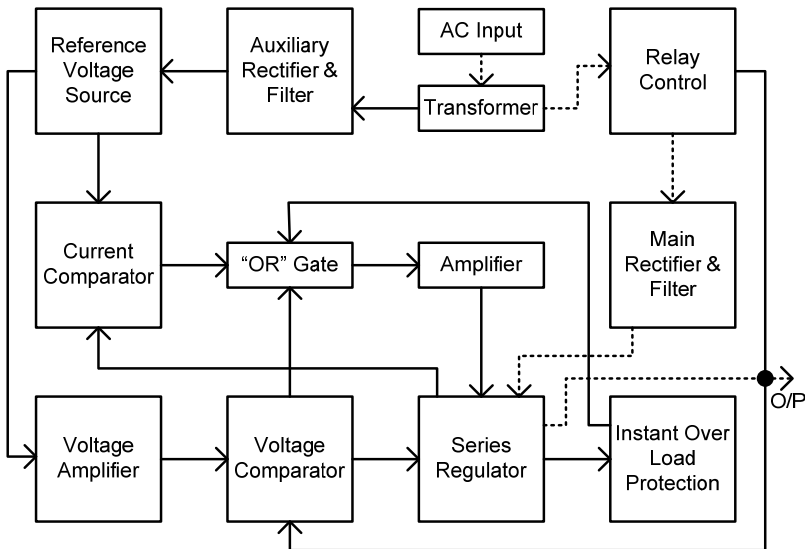

|                     |  |
|---------------------|--|
| Auxiliary Rectifier | The auxiliary rectifiers D1011~ D1014 provide bias voltage filtered by the capacitors C102 and C103, for the pre-regulators U101 and U102. They provide a regulated voltage for other modules.   |
| Main Rectifier      | The main rectifier is a full wave bridge rectifier. It provides the power after the rectifier is filtered by the capacitor C101, and then regulated via a series-wound regulator, which is finally delivered to the output terminal.   |
| Current Limiter     | U104 acts as a current limiter. When the current is over predetermined rating, U104 is activated and decreases the current. U208 provides a reference voltage. U206 is an inverter amplifier. U103 is a comparator amplifier which compares the reference voltage to the feedback voltage, and then delivers it to Q102, which then calibrates the output voltage. |
| Overload            | When the unit is overloaded, Q107 activates to control the current magnitude of Q102, to limit the output current. The relay control circuit controls the power dissipation in the series-wound regulated circuit.   |


## Front Panel Overview

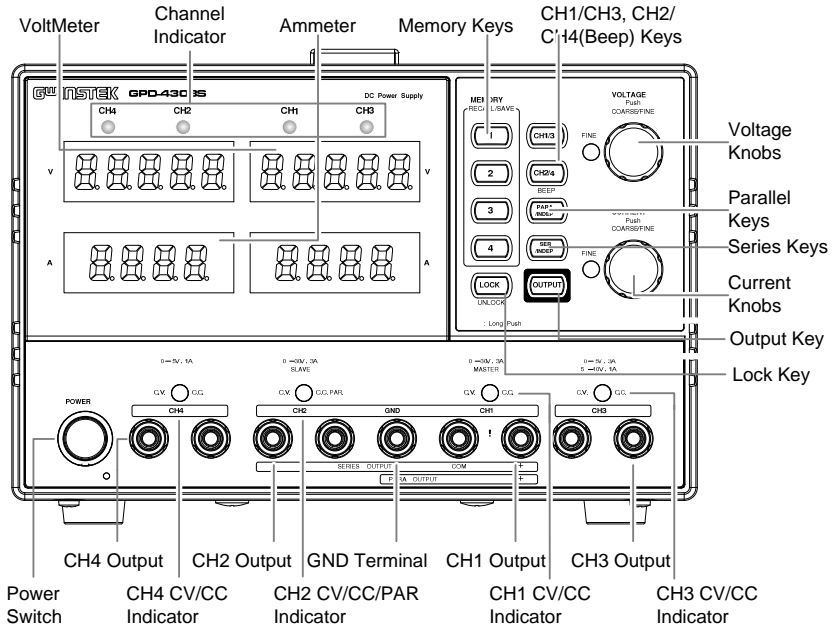

### Display


**Voltmeter** Displays output voltage of each channel.  
 GPD-4303S: CH1/CH3 and CH2/CH4  
 GPD-2303S/3303S: CH1 and CH2

5 digits:




**Ammeter** Displays output current of each channel.  
 GPD-4303S: CH1/CH3 and CH2/CH4  
 GPD-2303S/3303S: CH1 and CH2

4 digits:



Control Panel

Memory Keys



Saves or recalls panel settings. Four settings, 1 ~ 4, are available. For save/recall details, see page41.

CH1/CH2




GPD-2303S/2303S: Selects the output channel (CH1/CH2) for level adjustment. For level setting details, see page27.

CH1/3 and CH2/4



GPD-4303S: Selects the output channel (CH1/3 and CH2/4) for level adjustment. For level setting details, see page27.

Beep Keys



Pressing and holding the CH2 (2303S/3303S) or the CH2/4 key (4303S) enables the beeper sound. For details, see page25.

Parallel/Series Keys



Activates Tracking Parallel operation or Tracking Series operation, For details, see page33.

Lock Key




Locks or unlocks the front panel keys (excluding the OUTPUT key). Pressing the LOCK key will also exit remote mode if the machine is in remote mode. For details, see page26.

Output Key




Turns the output on or off.

Voltage Knobs




Adjusts the output voltage level for the selected channel. Pressing the knob switches coarse and fine level setting.

Current Knobs



Adjusts the output current level for the selected channel. Pressing the knob switches coarse and fine level setting.


Power Switch




Turns On  or Off  the main power. For power up sequence, see page 23.

Terminals


Default Terminals

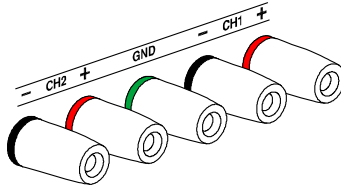

European Terminals

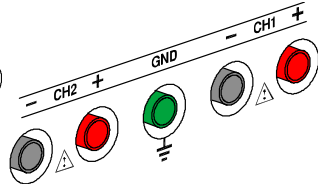


GND Terminal




Accepts a grounding wire.

CH1 CV/CC Indicator




Indicates CH1 Constant Voltage or Constant Current state.

CH1 Output




Outputs CH1 voltage and current.

CH2 CV/CC/PAR Indicator




Indicates CH2 Constant Voltage, Constant Current, or Tracking Parallel operation mode.

CH2 Output



Outputs CH2 voltage and current.

CH3 CV/CC Indicator



Indicates CH3 Constant Voltage or Constant Current state for the GPD-4303S.

CH3 Output




Outputs CH3 voltage and current.

CH3  
Overload  
Indicator




Indicates when CH3 (3303S) output current is overloaded.

CH3 Voltage  
Selector



Selects CH3 output voltage for the GPD-3303S: 2.5V, 3.3V, or 5V.

CH4 CV/CC  
Indicator




Indicates CH4 constant voltage or constant current for the GPD-4303S.

CH4 Output




Outputs CH4 voltage and current.

Channel  
Indicator



Indicates which channel the 2 LED voltmeters/ammeters represent.

# Rear Panel Overview

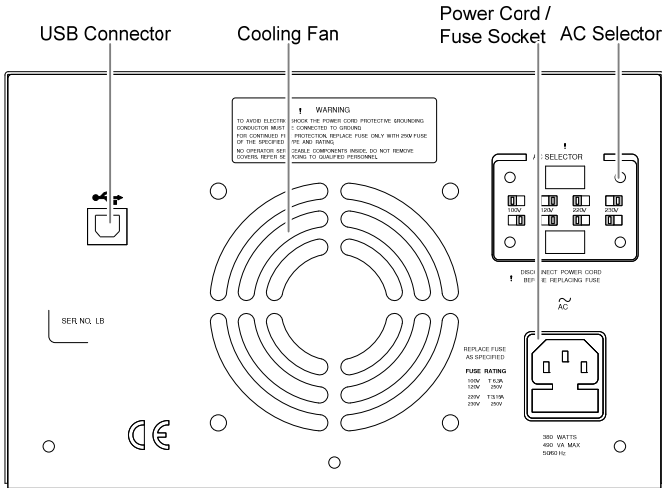


USB Connector



Accepts a USB slave connector for command-based remote control (page43).


Power Cord / Fuse Socket



The power cord socket accepts the AC mains: 115V/230V, 50/60Hz. For power up details, see page23.

The fuse holder contains the AC main fuse. For fuse replacement details, see page54.

AC Selector




Selects AC voltage: 100V/ 120V/ 220V/ 230V.

## CV/CC Crossover Characteristics

|            |  |
|------------|--|
| Background | The GPD-4303S, GPD-3303S and GPD-3303S automatically switch between constant voltage mode (CV) and constant current mode (CC), according to load condition.  |
| CV mode    | When <b>the current level is smaller than the output setting</b> , the GPD-X303S series operates in <b>Constant Voltage mode</b> . The indicator on the front panel turns green (C.V.) The Voltage level is kept at the setting and the Current level fluctuates according to the load condition until it reaches the output current setting.  |
| CC mode    | When <b>the current level reaches the output setting</b> , the GPD-X303S series starts operating in <b>Constant Current mode</b> . The indicator on the front panel turns red (C.C.) The Current level is kept at the setting but the Voltage level becomes lower than the setting, in order to suppress the output power level from overload. When the current level becomes lower than the setting, the GPD-X303S series goes back to the Constant Voltage mode. |

### Diagram

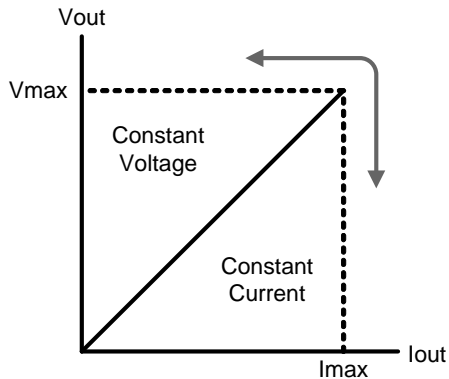


# SETUP


This chapter describes how to properly power up and configure the GPD-X303S series before operation.

## Power Up



**Select AC voltage** Before powering up the power supply, select the AC input voltage from the rear panel.



**Connect AC power cord** Connect the AC power cord to the rear panel socket.



**Power On** Press the Power switch to turn on the power. The display shows the initialization screen with the model name (3303S shown), followed by the last recalled settings.




**Power Off** Press the Power switch again to turn off the power.

## Load Cable Connection


GTL-104A

1. Turn the terminal counterclockwise and loosen the screw.
2. Insert the cable terminal.
3. Turn the terminal clockwise and tighten the screw.

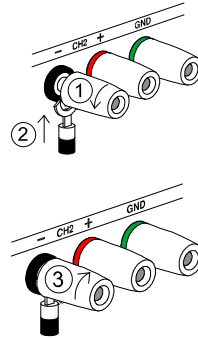


GTL-105A

Insert the plug into the socket.



GTL-203A, 204A

Insert the plug into the terminal.




Wire type

When using load cables other than the attached, make sure they have enough current capacity for minimizing cable loss and load line impedance. Voltage drop across a wire should not exceed 0.5V. The following list is the wire current rating at 450A/cm<sup>2</sup>.

| Wire size (AWG) | Maximum current (A) |
|-----------------|---------------------|
| 20              | 2.5                 |
| 18              | 4                   |
| 16              | 6                   |
| 14              | 10                  |
| 12              | 16                  |

## Output On/Off

Panel operation Pressing the Output key turns on all channel outputs.




The key LED also turns on. Pressing the Output key again turns the output and the key LED off.

Automatic output off Any of the following actions during output on automatically turns it off.

- Change the operation mode between independent / tracking series / tracking parallel
- Recalling other setups from the memory
- Storing the setup into the memory

## Beep On/Off

Panel operation By default, the beep sound is enabled. To turn off the beep, press the CH2 or CH2/CH4 key for 2 seconds.








A beep will be heard and the beep setting will be turned off. To enable the beep, press the CH2 or CH2/CH4 key again for 2 seconds.



List of beep The following operations beep when the beep setting is on.


- Power on
- INDEP - SER - PARA mode switching
- Setup save/recall
- Voltage/current knob fine/coarse switching
- Output on/off
- Panel lock/unlock
- CH1/CH2 output level knob switching
- Voltage/current level reaching minimum (zero) level

## Switch between channels

|                 |  |  |
|-----------------|--|--|
| Panel operation | <p>Switching between channels only applies to GPD-4303S.</p> <p>Press the CH1/3 key to toggle between CH1 and CH3. The active channel will be shown on the channel indicator.</p> <p>Press the CH2/4 key to toggle between CH2 and CH4. The active channel will be shown on the channel indicator.</p> | <p>CH4 CH2 CH1 CH3</p> <br><p>CH1/3</p> <br><p>CH1 CH3</p> <br><p>CH2/4</p> <br><p>CH4 CH2</p>  |
|-----------------|--|--|

## Front Panel Lock


|                 |   |  |
|-----------------|---|--|
| Panel operation | <p>Press the LOCK key to lock the front panel key operation. The key LED turns on. To unlock, press the LOCK key for 2 seconds. The key LED also turns off.</p> |  <span style="font-size: 2em;">→</span>  |
|-----------------|---|--|

|      |  |  |
|------|--|--|
| Note | <p>The OUTPUT key is not affected by the lock operation.</p> |  |
|------|--|--|

# OPERATION



## CH1/CH2 Independent Mode

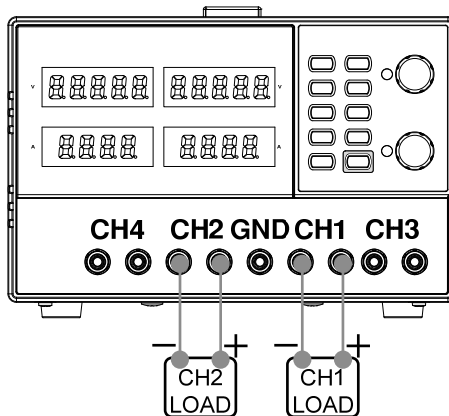
Background / Connection CH1 and CH2 outputs work independent of each other.



Output rating 0 ~ 30V/0~3A for each channel

- Panel operation
1. Make sure the PARA/INDEP and SER/INDEP keys are turned off (the key LEDs are off).
 



  

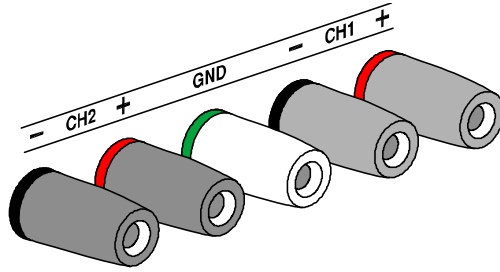  2. Connect the load to the front panel terminals, CH1 +/-, CH2 +/-.



Note: this diagram shows non-European terminals.

- Set the CH1 output voltage (For CH1) and current. Press the CH1 key (LED turns on) and then use the Voltage and Current knob.



By default, the Voltage and Current knob work in the coarse mode. To activate the fine mode, press the knob to (Fine control) turn the FINE LED on.



- Coarse: 0.1V or 0.1A for each step
- Fine: 1mV or 1mA for each step


- Repeat the above settings for the CH2.

- To turn on the output, press the output key. The key LED turns on and the CH1 / CH2 indicator shows the output mode, CV or CC.



## CH3 Independent Mode


Background / Connection For the GDP-3303S the CH3 rating is fixed at 2.5V/3.3V/5V, 3A. CH3 for the 4303S is variable: 0~5V,0~3A / 5.001~10V,0~1A .

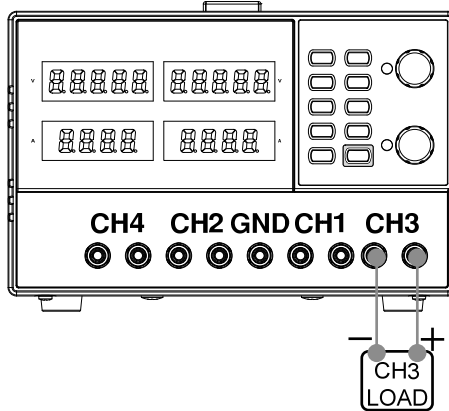


Output rating 3303S : 2.5V/3.3V/5V, 3A (fixed)  
4303S : 0~5V,0~3A / 5.001~10V,0~1A

No Tracking Series/Parallel CH3 does not have tracking series/parallel mode. Also, CH3 output is not affected by CH1 and CH2 modes.

Panel operation 1. Connect the load to the front panel CH3 +/- terminal. (the diagram shows non-European terminals)




2. 3303S: Select the output voltage, 2.5V/3.3V/5V using the CH3 voltage selector key.



4303S: Press the CH1/3 key to switch to CH3 (The CH3 indicator will light). Use the voltage and current knobs to set the voltage and current.




3. To turn on the output, press the output key. The key LED turns on.




CV → CC

3303S: When the output Current level exceeds 3.2A, the overload indicator turns red and CH3 operation mode switches from Constant Voltage to Constant Current.



4303S: When the output value exceeds the set value, the C.V./C.C. indicator turns red. This indicates that CH3 has switched from the constant voltage to constant current.




Note

Note: “overload” on CH3 in this case does not mean an abnormal operation.

# CH4 Independent Mode


Background / Connection      The GPD-4303S has a rating of 5V/1A max.

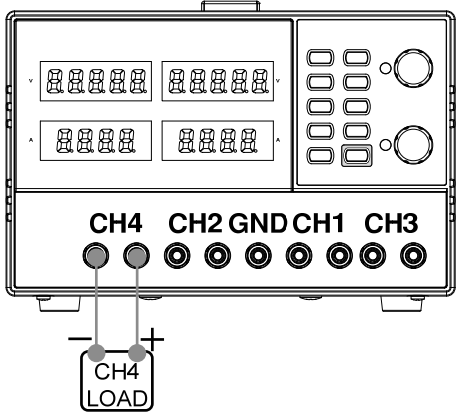

Output rating      5V/1A max

No Tracking      CH4 does not have tracking series/parallel mode.  
Series/Parallel      The CH4 output is not affected by CH1 and CH2 modes.


Panel operation      1. Connect the load to the front panel CH4 +/- terminal. (the diagram shows non-European terminals)



2. Press the CH2/4 key to switch to CH4 (The CH4 indicator will light). Use the voltage and current knobs to set the voltage and current.




3. To turn on the output, press the output key. The key LED turns on.



CV → CC

When the output value exceeds the set value, the C.V./C.C. indicator turns red. This indicates that CH3 has switched from constant voltage to constant current.




## CH1/CH2 Tracking Series Mode

**Background** Tracking series operation doubles the Voltage capacity of the GPD-X303S series by internally connecting CH1 (Master) and CH2 (Slave) in series and combining the output to a single channel. CH1 (Master) controls the combined Voltage output level.

The following describes two types of configurations depending on the common ground usage.


### Tracking series without common terminal


**Connection**

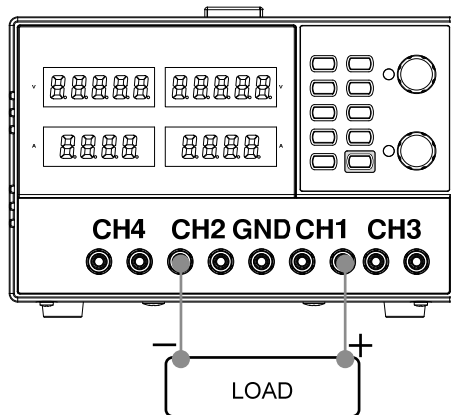

**Output rating** 0 ~ 60V/0 ~ 3A


1. Press the SER/INDEP key to activate the tracking series mode. The key LED turns on.
2. Connect the load to the front panel terminals, CH1+ & CH2- (Single supply).



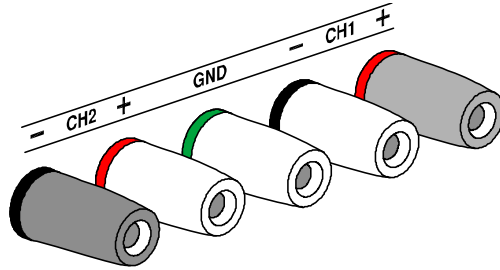


Note: this diagram shows non-European terminals.


3. Press the CH2 key (LED turns on) and then use the Current knob to set the CH2 output current to the maximum level (3.0A). By default, the Voltage and Current knob work in the coarse mode. To activate the fine mode, press the knob to turn the FINE LED on.



CURRENT  
Push  
COARSE/FINE




(Fine control)




- Coarse: 0.1V or 0.1A for each step
- Fine: 1mV or 1mA for each step


4. Press the CH1 key (LED turns on) and then use the Voltage and Current knob to set the output voltage and current level.




VOLTAGE  
Push  
COARSE/FINE




CURRENT  
Push  
COARSE/FINE



5. To turn on the output, press the output key. The key LED turns on.



6. Refer to the CH1 (Master) meter and indicator for the output setting level and CV/CC status.

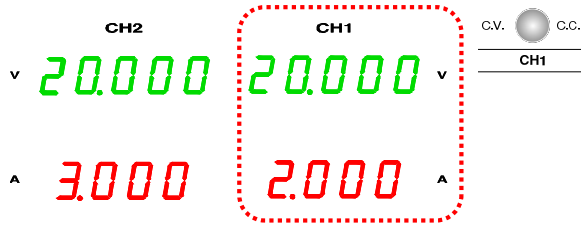


**Voltage level** Double the reading on the CH1 Voltage meter. In the above case, the actual output is  $20.0 \times 2 = 40.0V$ .


**Current level** CH1 meter reading shows the output Current. In the above case, 2.000A. (CH2 Current control must be in the Maximum position=3.0A).


### Tracking series with common terminal

Connection

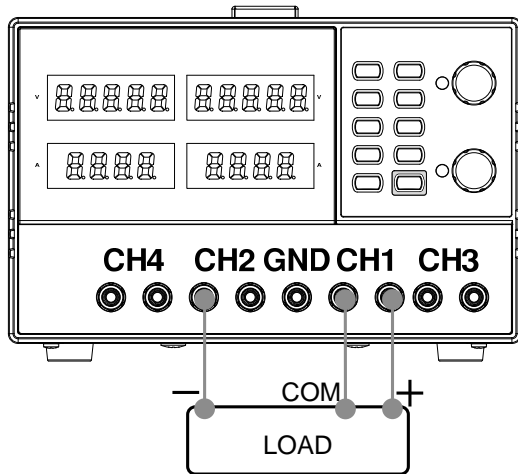


**Output rating** 0~30V/0~3A for CH1 ~ COM  
 0~-30V/0~3A for CH2 ~ COM


1. Press the SER/INDEP key to activate the tracking series mode. The key LED turns on. 
2. Connect the load to the front panel terminals, CH1+ & CH2-. Use the CH1 (-) terminal as the common line connection.

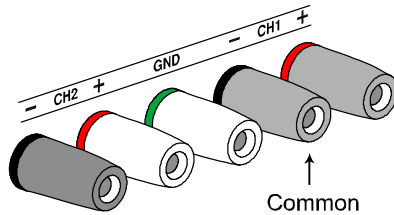


Note: this diagram shows non-European terminals.

3. Press the CH1 key (LED turns on) and use the Voltage knob to set the master & slave output voltage (the same level for both channels). By default, the Voltage and Current knob work in the coarse mode. To activate the fine mode, press the knob to turn the FINE LED on. 


(master & slave)




(Fine control)




- Coarse: 0.1V or 0.1A for each step
  - Fine: 1mV or 1mA for each step
4. Use the Current knob to set the master output current.



5. To turn on the output (and LED), press the output key.




6. For the master (CH1) output level and CV/CC status, refer to the CH1 meter and indicator.

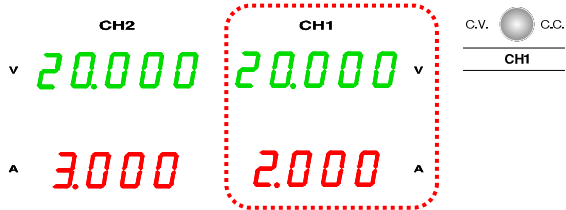


Master (CH1) CH1 meter reading shows the voltage level  
 output level In the above case, 20.0V.

Master (CH1) CH1 meter reading shows the current level  
 output current. In the above case, 2.000A.

7. Press the CH2 key (LED turns on) and use the Current knob to set the slave output current.



8. For the slave (CH2) output level and CV/CC status, refer to the CH1/CH2 meter and CH2 indicator.

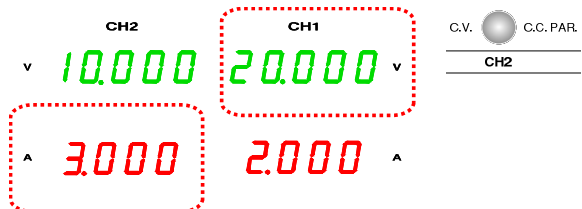


|                              |  |
|------------------------------|--|
| Slave (CH2)<br>voltage level | The CH1 meter reading shows the output voltage. In the above case, 20.0V.  |
| Slave (CH2)<br>current level | The CH2 meter reading shows the output current. In the above case, 3.000A. |

## CH1/CH2 Tracking Parallel Mode


Background /  
Connection

Tracking parallel operation doubles the current capacity of the GPD-X303S series by internally connecting CH1 and CH2 in parallel and combining the output to a single channel. CH1 controls the combined output.

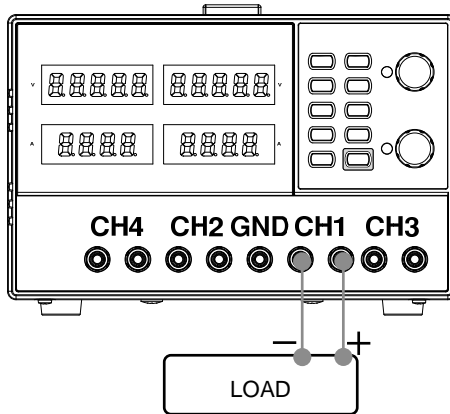


Output rating 0 ~ 30V/0 ~ 6A

1. Press the PARA/INDEP key to activate the tracking parallel mode. The key LED turns on.




2. Connect the load to the CH1 +/- terminals.

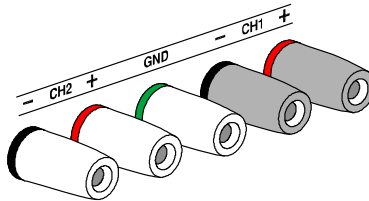


Note: this diagram shows non-European terminals.


3. To turn on the output, press the output key. The key LED turns on.




4. The CH2 C.V./C.C. PAR. indicator turns red, indicating tracking parallel (PARA) mode.



5. Press the CH1 key (LED turns on) and then use the Voltage and Current knob to set the output voltage and current. The CH2 output control is disabled. By default, the Voltage and Current knob work in the coarse mode. To activate the fine mode, press the knob to turn the FINE LED on.

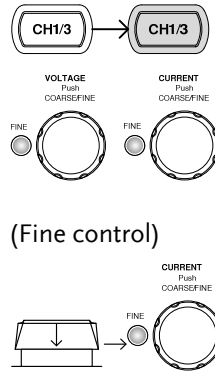

6. For the output level and CV/CC status, refer to the CH1 meter and indicator.

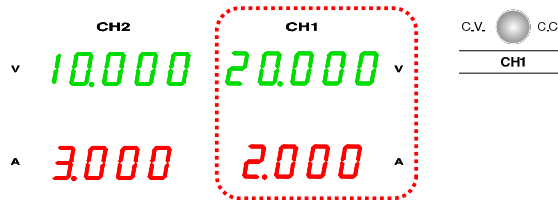

Voltage level The CH1 meter reading shows the output voltage. In the above case, 20.0V.

Current level Double the amount of CH1 current meter reading. In the above case,  $2.0A \times 2 = 4.0A$ .

# SAVE/RECALL SETUP

## Save Setup

**Background** The front panel settings can be stored into one of the four internal memories.


**Contents** The following list shows the setup contents.

- Independent / tracking series / tracking parallel mode
- CH1/CH2 knob selection
- Fine/coarse editing mode
- Output voltage/current level

The following settings are always saved as “off”.

- Output on/off
- Front panel lock/unlock
- Buzzer on/off

**Panel operation** Press one of the 1~4 Memory keys for 2 seconds, for example memory 1. The panel settings are saved in memory 1 and the key LED turns on. When the panel settings are modified, the LED turns off.



**Note** When a setting is stored, the output automatically turns off.

## Recall Setup

**Background** The front panel settings can be recalled from one of the four internal memories.


**Contents** The following list shows the setup contents.

- Independent / tracking series / tracking parallel mode
- CH1/CH2 knob selection
- Fine/coarse editing mode
- Output voltage/current level

The following settings are always recalled as “off”.

- Output on/off
- Front panel lock/unlock
- Buzzer on/off


**Panel operation** Press one of the 1~4 Memory keys, for example memory 1. The panel settings saved in memory 1 are recalled. The key LED turns on. When the panel settings are modified, the LED turns off.



**Note** When a setting is recalled, the output automatically turns off.

# RREMOTE CONTROL


## Remote Control Setup

|                     |  |                            |
|---------------------|--|----------------------------|
| Background          | The GPD-X303S is capable of being remotely controlled via a USB connection.  |                            |
| Interface           |   | USB slave port, rear panel |
| COM setting         | <p>Set up the COM port inside the PC according to the following list.</p> <ul style="list-style-type: none"> <li>• Baud rate: 9600/57600 /115200</li> <li>• Parity bit: None</li> <li>• Data bit: 8</li> <li>• Stop bit: 1</li> <li>• Data flow control: None</li> </ul>         |                            |
| Functionality check | <p>Run this query command via the terminal application such as MTTY (Multi-threaded TTY).</p> <p>*IDN?</p> <p>This should return the identification information: Manufacturer, model name, serial number, firmware version.</p> <p>GW INSTEK, GPD-x303S, SN: xxxxxxxx, Vx.xx</p> |                            |


## Remote Connection Step

Entering the remote control mode

1. Connect the USB cable to the slave port.
2. The connection will be automatically established, and the front panel shows a "USB...YES" message.

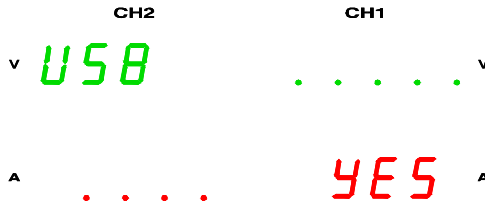


3. The power supply front panel is automatically locked (the Lock key will become activated).




Leaving the remote control mode

1. To exit remote mode either, 1) use the LOCAL command from the terminal connection, or 2) Press the LOCK key on the front panel to return to local mode, or 3) disconnect the USB cable from the rear panel.
2. The display shows "USB...NO" message.

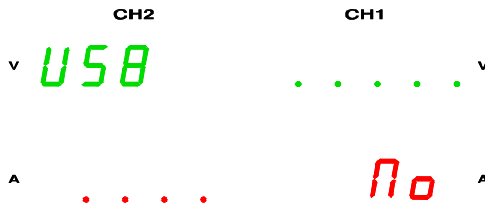

3. The LOCK will no longer be lit when remote mode is off.



4. The power supply goes back to the local operation mode.

## Command Syntax

Command format **ISET<X>:<NR2>NL** 1: command header  
 2: output channel  
 3: separator  
 4: parameter  
 5: terminator(line feed)

Output channel 1 (CH1) or 2 (CH2)

| Parameter | Type | Description     | Example         |
|-----------|------|-----------------|-----------------|
| <Boolean> |      | boolean logic   | 0 (off), 1 (on) |
| <NR1>     |      | integers        | 0, 1, 2, 3      |
| <NR2>     |      | decimal numbers | 0.1, 3.14, 8.5  |

Terminator Each command must end with a terminal character (new line code, ASCII: 0x0A) and each query must end with a carriage return, ASCII: 0x0D.

Note Commands are not case-sensitive.

## Error Messages

The following error messages might appear when the GPD-X303S cannot accept the command.

| Message contents            | Descriptions   |
|-----------------------------|--|
| a Program mnemonic too long | The command length must be 15 characters or less.                                |
| b Invalid character         | Invalid characters, such as symbols, are entered. Example: VOUT#                 |
| c Missing parameter         | The parameter is missing from the command. Example: VSET: (should have a number) |
| d Data out of range         | The entered value exceeds the specification. Example: VSET:33 (should be ≤ 32V)  |

|   |                     |   |
|---|---------------------|---|
| e | Command not allowed | The entered command is not allowed in the circumstance. Example: trying to set CH2 output while in the tracking mode. |
| f | Undefined header    | The entered command does not exist, or the syntax is wrong.   |

## Command List

- Detailed descriptions of each command start from the next page.
- The “HELP” command shows all the below commands and their meanings, except for the HELP command itself.

|               |  |
|---------------|--|
| ISET<X>:<NR2> | Sets the output current.               |
| ISET<X>?      | Returns the output current setting.    |
| VSET<X>:<NR2> | Sets the output voltage.               |
| VSET<X>?      | Returns the output voltage setting.    |
| IOUT<X>?      | Returns the actual output current.     |
| VOUT<X>?      | Returns the actual output voltage.     |
| TRACK<NR1>    | Selects the operation mode.            |
| BEEP<BOOLEAN> | Turn on or off the beep.               |
| OUT<BOOLEAN>  | Turn on or off the output.             |
| STATUS?       | Returns the GPD-X303S status.          |
| *IDN?         | Returns the GPD-X303S identification.  |
| RCL<NR1>      | Recalls a panel setting.               |
| SAV<NR1>      | Saves the panel setting.               |
| HELP?         | Shows the command list.                |
| ERR?          | Returns the instrument error messages. |
| BAUD<NR1>     | Sets the baud rate.                    |
| LOCAL         | Returns the instrument to local mode.  |

## Command Details

### ISET<X>:<NR2>

|               |   |  |
|---------------|---|--|
| Description   | Sets the output current for the selected channel. |  |
| X             | 1= CH1, 2= CH2, (4303S: 3 = CH3, 4= CH4)          |  |
| <NR2>         | Decimal number, range 0~3.200A                    |  |
| Response time | Minimum 10ms                                      |  |
| Example       | ISET1:2.234                                       | Sets the CH1 output current to 2.234A. |

### ISET<X>?

|               |  |   |
|---------------|--|---|
| Description   | Returns the output current setting.      |   |
| X             | 1= CH1, 2= CH2, (4303S: 3 = CH3, 4= CH4) |   |
| Response time | Minimum 10ms                             |   |
| Example       | ISET1?                                   | Returns the CH1 output current setting. |

### VSET<X>:<NR2>

|               |   |                                 |
|---------------|---|---------------------------------|
| Description   | Sets the output voltage.                |                                 |
| X             | 1: CH1, 2: CH2, (4303S: 3: CH3, 4: CH4) |                                 |
| <NR2>         | Decimal number, range 0~32.000V         |                                 |
| Response time | Minimum 10ms                            |                                 |
| Example       | VSET1:20.345                            | Sets the CH1 voltage to 20.345V |

### VSET<X>?

|               |   |                                 |
|---------------|---|---------------------------------|
| Description   | Returns the output voltage setting.     |                                 |
| X             | 1: CH1, 2: CH2, (4303S: 3: CH3, 4: CH4) |                                 |
| Response time | Minimum 10ms                            |                                 |
| Example       | VSET1?                                  | Returns the CH1 voltage setting |

### IOUT<X>?

|               |   |                                |
|---------------|---|--------------------------------|
| Description   | Returns the actual output current.      |                                |
| X             | 1: CH1, 2: CH2, (4303S: 3: CH3, 4: CH4) |                                |
| Response time | Minimum 10ms                            |                                |
| Example       | IOUT1?                                  | Returns the CH1 output current |

### VOUT<X>?

|               |   |                                |
|---------------|---|--------------------------------|
| Description   | Returns the actual output voltage.      |                                |
| X             | 1: CH1, 2: CH2, (4303S: 3: CH3, 4: CH4) |                                |
| Response time | Minimum 10ms                            |                                |
| Example       | VOUT1?                                  | Returns the CH1 output voltage |

### TRACK<NR1>

|               |   |                              |
|---------------|---|------------------------------|
| Description   | Selects the operation mode: independent, tracking series, or tracking parallel. |                              |
| NR1           | 0: Independent, 1: Series, 2: Parallel  |                              |
| Response time | Minimum 10ms  |                              |
| Example       | TRACK0  | Selects the independent mode |

### BEEP<Boolean>

|               |                           |                   |
|---------------|---------------------------|-------------------|
| Description   | Turns the beep on or off. |                   |
| <Boolean>     | 0:off, 1:on               |                   |
| Response time | Minimum 10ms              |                   |
| Example       | BEEP1                     | Turns on the beep |

### OUT<Boolean>

|               |                             |                     |
|---------------|-----------------------------|---------------------|
| Description   | Turns on or off the output. |                     |
| <Boolean>     | 0: off, 1: on               |                     |
| Response time | Minimum 10ms                |                     |
| Example       | OUT1                        | Turns on the output |

### STATUS?

|               |                         |  |
|---------------|-------------------------|--|
| Description   | Returns the GPD-X3303S. |  |
| Response time | Minimum 10ms            |  |

Return parameter 8 bits in the following format

| Bit  | Item     | Description  |
|------|----------|--|
| 0    | CH1      | 0=CC mode, 1=CV mode                                     |
| 1    | CH2      | 0=CC mode, 1=CV mode                                     |
| 2, 3 | Tracking | 01=Independent, 11=Tracking series, 10=Tracking parallel |
| 4    | Beep     | 0=Off, 1=On  |
| 5    | Output   | 0=Off, 1=On  |
| 6, 7 | Baud     | 00=115200bps, 01=57600bps, 10=9600bps                    |

### \*IDN?

|               |  |  |
|---------------|--|--|
| Description   | Returns the instrument identification. |  |
| Response time | Minimum 10ms                           |  |

Return parameter GW INSTEK,GPD-X3303,SN: xxxxxxxx, Vx.xx  
(Manufacturer, model name, serial number,  
firmware version)

### RCL<NR1>

|               |                          |  |
|---------------|--------------------------|--|
| Description   | Recalls a panel setting. |  |
| <NR1>         | 1 - 4: Memory 1 to 4     |  |
| Response time | Minimum 10ms             |  |
| Example       | RCL1                     | Recalls the panel setting stored in memory 1 |

### SAV<NR1>

|               |                           |                                      |
|---------------|---------------------------|--------------------------------------|
| Description   | Stores the panel setting. |                                      |
| <NR1>         | 1 - 4: Memory 1 to 4      |                                      |
| Response time | Minimum 10ms              |                                      |
| Example       | SAV1                      | Stores the panel setting in memory 1 |

### BAUD<NR1>

|               |  |                                  |
|---------------|--|----------------------------------|
| Description   | Sets the baud rate to 9600bps/57600bps /115200bps. |                                  |
| <NR1>         | 0: 115200bps, 1: 57600bps, 2: 9600bps              |                                  |
| Response time | Minimum 10ms                                       |                                  |
| Example       | BAUD0  | Sets the baud rate to 115200bps. |

### LOCAL

|             |  |  |
|-------------|--|--|
| Description | Exits remote mode and sets the instrument to local mode. |  |
|-------------|--|--|

|               |              |
|---------------|--------------|
| Response time | Minimum 10ms |
|---------------|--------------|

## ERR?

|             |   |
|-------------|---|
| Description | Checks the error status of the instrument and returns the last error message. |
|-------------|---|

|               |              |
|---------------|--------------|
| Response time | Minimum 10ms |
|---------------|--------------|

|          |   |
|----------|---|
| Contents | See page 46 for the list of error messages. |
|----------|---|

## HELP?

|             |                         |
|-------------|-------------------------|
| Description | Shows the command list. |
|-------------|-------------------------|

|               |              |
|---------------|--------------|
| Response time | Minimum 50ms |
|---------------|--------------|

|                   |   |
|-------------------|---|
| Return parameters | <p>                     ISET&lt;x&gt;:&lt;NR2&gt; Sets the value of current.<br/>                     VSET&lt;x&gt;:&lt;NR2&gt; Sets the value of voltage.<br/>                     ISET&lt;x&gt; ? Return the value of current.<br/>                     VSET&lt;x&gt; ? Return the value of voltage.<br/>                     IOUT&lt;x&gt; ? Returns actual output current ,<br/>                     VOUT&lt;x&gt; ? Returns actual output voltage.<br/>                     TRACK&lt;NR1&gt; Sets the output of the power supply working on independent or tracking mode.<br/>                     BAUD&lt; NR1 &gt;Set the value of baud rate.<br/>                     RCL&lt;NR1&gt; Recall the setting data from the memory which previous saved.<br/>                     SAV&lt;NR1&gt; Saves the setting data to memory.<br/>                     BEEP&lt;Boolean&gt; Sets the BEEP state on or off.<br/>                     OUT&lt;Boolean&gt; Sets the output state on or off.<br/>                     LOCAL Return to local mode<br/>                     *IDN ? Returns instrument identification.<br/>                     ERR ? Returns instrument error messages.<br/>                     STATUS ? Returns the power supply state.                 </p> |
|-------------------|---|



Note

All response time estimates are based on a baud rate of 115200bps. Expect longer response times with a baud rate of 57600bps or 9600bps.

# F AQ

Q1. I pressed the panel lock key but the output still turns on/off.

---

A1. For safety reasons the output key is not affected by the panel key lock feature.

Q2. The CH3 overload indicator turned on – is this an error?

---

A2. No, it simply means that the CH3 output current reached the maximum 3.0A and the operation mode turned from CV (constant voltage) to CC (constant current). You can continue using the power supply, although reducing the output load is recommended.

Q3. The specifications do not match the real accuracies.

---

A3. Make sure that the power supply is powered on for at least 30 minutes, within +20°C – +30°C.

Q4. The internal memory is not recording the panel setting correctly – the output should be on.

---

A4. The output is always stored or recalled as “off” to ensure safety.

For more information, contact your local dealer or GWInstek at [www.gwinstek.com.tw](http://www.gwinstek.com.tw) / [marketing@goodwill.com.tw](mailto:marketing@goodwill.com.tw).


# APPENDIX

## Fuse Replacement


---

### Steps

1. Take off the power cord and remove the fuse socket using a minus driver.

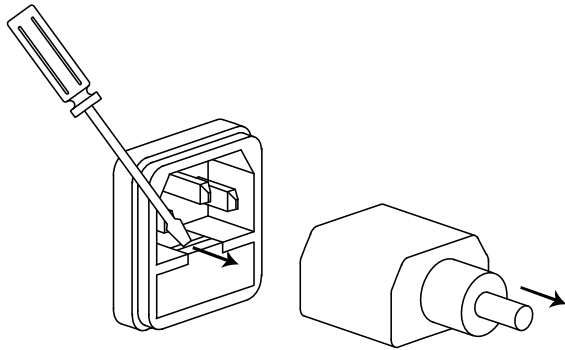

2. Replace the fuse in the holder.

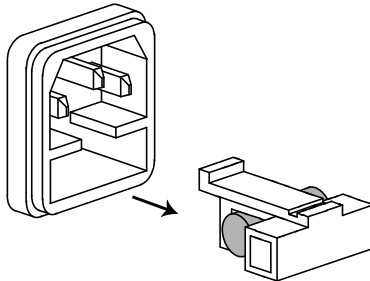

### Rating

- 100V/120V:T6.3A/250V
- 220V/230V:T3.15A/250V

## Specifications

The specifications apply when the GPD-X303S series are powered on for at least 30 minutes under +20°C – +30°C.

|                    |                         |   |
|--------------------|-------------------------|---|
| Output Ratings     | CH1/CH2 Independent     | 0 ~ 30V / 0 ~ 3A  |
|                    | CH1/CH2 Series          | 0 ~ 60V / 0 ~ 3A  |
|                    | CH1/CH2 Parallel        | 0 ~ 30V / 0 ~ 6A  |
|                    | CH3                     | 2.5V/3.3V/5.0V, 0 ~ 3A(3303S)<br>0~5V,0~3A / 5.001~10V,0~1A(4303S)  |
| Voltage Regulation | CH4                     | 0~5V,0~1A   |
|                    | Line                    | $\leq 0.01\% + 3\text{mV}$  |
|                    | Load                    | $\leq 0.01\% + 3\text{mV}$ (rating current $\leq 3\text{A}$ )<br>$\leq 0.02\% + 5\text{mV}$ (rating current $> 3\text{A}$ )   |
|                    | Ripple & Noise          | $\leq 1\text{mVrms}$ (5Hz ~ 1MHz)   |
|                    | Recovery Time           | $\leq 100\mu\text{s}$ (50% load change, minimum load 0.5A)  |
| Current Regulation | Temperature Coefficient | $\leq 300\text{ppm}/^\circ\text{C}$   |
|                    | Line                    | $\leq 0.2\% + 3\text{mA}$   |
|                    | Load                    | $\leq 0.2\% + 3\text{mA}$   |
| Tracking Operation | Ripple & Noise          | $\leq 3\text{mArms}$  |
|                    | Tracking Error          | $\leq 0.1\% + 10\text{mV}$ of Master (0~30V)<br>(No Load, with load add load regulation $\leq 100\text{mV}$ )   |
|                    | Parallel Regulation     | Line: $\leq 0.01\% + 3\text{mV}$<br>Load: $\leq 0.01\% + 3\text{mV}$ (rating current $\leq 3\text{A}$ )<br>Load: $\leq 0.02\% + 5\text{mV}$ (rating current $> 3\text{A}$ ) |
| Meter Resolution   | Series Regulation       | Line: $\leq 0.01\% + 5\text{mV}$<br>Load: $\leq 100\text{mV}$   |
|                    | Voltage and current     | Voltage: 1mV<br>Current: 1mA  |
| Resolution         | Ammeter                 | 3.2A full scale, 4 digits 0.4" LED display  |

|                       |  |   |
|-----------------------|--|---|
|                       | Voltmeter  | 32V full scale, 5 digits 0.4" LED display                                   |
| Program               |  | Voltage: $\pm (0.03\% \text{ of reading} + 10\text{mV})$                    |
| Accuracy              |  | Current: $\pm (0.3\% \text{ of reading} + 10\text{mA})$                     |
| Read back             |  | Voltage: $\pm (0.03\% \text{ of reading} + 10\text{mV})$                    |
| Accuracy              |  | Current: $\pm (0.3\% \text{ of reading} + 10\text{mA})$                     |
| CH3 of 3303S          | Voltage  | 2.5V/3.3V/5.0V, $\pm 5\%$   |
|                       | Current  | 3A  |
|                       | Line   | $\leq 3\text{mV}$   |
|                       | Load   | $\leq 5\text{mV}$   |
|                       | Ripple & Noise   | $\leq 1\text{mVrms}$ (5Hz ~ 1MHz)   |
| Insulation            | Chassis and Terminal   | 20M $\Omega$ or above (DC 500V)   |
|                       | Chassis and AC cord  | 30M $\Omega$ or above (DC 500V)   |
| Operation Environment | Indoor use, Altitude: $\leq 2000\text{m}$<br>Ambient temperature: 0 ~ 40°C<br>Relative humidity: $\leq 80\%$<br>Installation category: II, Pollution degree: 2 |   |
| Storage Environment   | Ambient temperature: -10 ~ 70°C<br>Relative humidity: $\leq 70\%$  |   |
| Power Source          | AC 100V/120V/220V/230V $\pm 10\%$ , 50/60Hz  |   |
| Accessories           | User manual  | x1  |
|                       | Test lead  | GTL-104A x 2, GTL-105A x 1<br>(Europe) Test lead GTL-203A x 1, GTL-204A x 2 |
| Dimensions            | 210 (W) x 130 (H) x 265 (D) mm   |   |
| Weight                | Approx. 7kg  |   |

## Options

|           |         |                   |
|-----------|---------|-------------------|
| USB cable | GTL-246 | USB 2.0, A-B type |
|-----------|---------|-------------------|

## Declaration of Conformity

We

**COMBINED TEST SOLUTIONS**

(1)

**Type of Product: Power Supply**

**Model Number: GPD-2303S/ GPD-3303S / GPD-4303S**

are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (2004/108/EC) and Low Voltage Directive (2006/95/EC).

For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

### © EMC

|   |        |                                |
|---|--------|--------------------------------|
| EN 61326-1: 2006 Electrical equipment for measurement, control and laboratory use -- EMC requirements |        |                                |
| Conducted Emission  | ClassB | Electrostatic Discharge        |
| Radiated Emission   |        | EN 61000-4-2: 2008             |
| EN 55011: 2009 + A1: 2010   |        | Radiated Immunity              |
|   |        | EN 61000-4-3: 2006+A2:2010     |
| Current Harmonics   |        | Electrical Fast Transients     |
| EN 61000-3-2: 2006+A2:2009  |        | EN 61000-4-4: 2004+A1:2010     |
| Voltage Fluctuations  |        | Surge Immunity                 |
| EN 61000-3-3: 2008  |        | EN 61000-4-5: 2005             |
| -----   |        | Conducted Susceptibility       |
|   |        | EN 61000-4-6:2008              |
| -----   |        | Power Frequency Magnetic Field |
|   |        | EN 61000-4-8: 2009             |
| -----   |        | Voltage Dip/ Interruption      |
|   |        | EN 61000-4-11: 2004            |

### © Safety

|  |
|--|
| Low Voltage Equipment Directive 2006/95/EC |
| Safety Requirements                        |
| IEC/EN 61010-1: 2001(Second Edition)       |

# INDEX

|                              |        |                               |        |
|------------------------------|--------|-------------------------------|--------|
| Automatic out off .....      | 25     | Operation.....                | 7      |
| Banana plug .....            | 24     | Specification .....           | 55     |
| Baud rate                    |        | Storage.....                  | 8      |
| Remote control.....          | 51     | Error messages, remote        |        |
| Beep setting                 |        | control .....                 | 46, 52 |
| Contents.....                | 25     | Front panel                   |        |
| Manual.....                  | 25     | Lock (manual) .....           | 26     |
| Remote control.....          | 50     | Overview .....                | 16     |
| Caution symbol .....         | 5      | Fuse                          |        |
| CC/CV.....                   | 30     | Rating .....                  | 55     |
| CC/CV indicator .....        | 32     | Replacement.....              | 54     |
| Cleaning the instrument..... | 7      | Safety instruction.....       | 7      |
| COM setting, remote control  |        | GPD series                    |        |
| .....                        | 43     | Block diagram .....           | 14     |
| Command list .....           | 47     | Dynamic load .....            | 12     |
| Recalling the list .....     | 52     | List of features.....         | 13     |
| Common terminal, tracking    |        | Operation theory .....        | 14     |
| series.....                  | 33     | Technology overview.....      | 10     |
| Cooling fan.....             | 21     | Ground symbol .....           | 5      |
| safety instruction.....      | 6      | Identification information .. | 50     |
| CV/CC                        |        | Load connection.....          | 24     |
| CH1/CH2 indicator .....      | 28     | Local                         |        |
| CH3 indicator.....           | 30     | Remote control .....          | 51     |
| CH4 indicator.....           | 32     | Operation mode                |        |
| Operation theory .....       | 11, 22 | Independent .....             | 27     |
| Disposal instructions .....  | 8      | Specifications.....           | 55     |
| EN61010                      |        | Tracking parallel.....        | 39     |
| Declaration of conformity    | 57     | Tracking series .....         | 33     |
| Measurement category .....   | 6      | Output current setting        |        |
| Pollution degree .....       | 8      | Manual .....                  | 28     |
| EN61326-1 .....              | 57     | Remote control.....           | 48     |
| Environment                  |        | Output on/off                 |        |

|                               |    |                         |    |
|-------------------------------|----|-------------------------|----|
| FAQ .....                     | 53 | Command syntax.....     | 46 |
| manual .....                  | 25 | Connection test.....    | 43 |
| Remote .....                  | 50 | Error messages .....    | 46 |
| Output voltage setting        |    | Interface.....          | 43 |
| Manual .....                  | 28 | Save settings           |    |
| Remote control.....           | 48 | Manual .....            | 41 |
| Over load indicator .....     | 30 | Remote.....             | 51 |
| Power supply                  |    | Service operation       |    |
| Safety instruction.....       | 6  | About disassembly ..... | 6  |
| Setup .....                   | 23 | Contact .....           | 53 |
| Socket overview.....          | 21 | Status, instrument..... | 50 |
| Specification .....           | 55 | Switch channels.....    | 26 |
| Protective ground symbol..... | 5  | Tracking mode           |    |
| Rear panel overview .....     | 21 | Operation theory.....   | 11 |
| Recall settings               |    | UK power cord.....      | 9  |
| Manual .....                  | 42 | USB interface .....     | 43 |
| Remote .....                  | 51 | Warning symbol.....     | 5  |
| Remote control                |    | Wire, load.....         | 24 |

Combined Test Solutions,  
4 Commerce Way, Stanbridge Road,  
Leighton Buzzard, LU7 4RW

T: 01525 374466  
E: [sales@ctstest.co.uk](mailto:sales@ctstest.co.uk)  
W: [www.ctstest.co.uk](http://www.ctstest.co.uk)

